
Weqas
Unit 6, Parc Tŷ Glas,
Llanishen
Cardiff, UK
CF14 5DU
Tel: +44 (0) 2920 314750
E-mail: office@weqas.com

UKAS PROFICIENCY TESTING 4301

POCT INR CueSee Coag
Sample Instructions

OPERATING PROCEDURE:

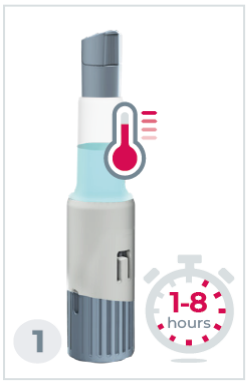


Place vial at room temperature for at least 1 hour but not longer than 8 hours before testing.



To activate hold the white section and turn the grey section 180 degrees until the long indents align.



Immediately shake vigorously and continuously for 1 minute.

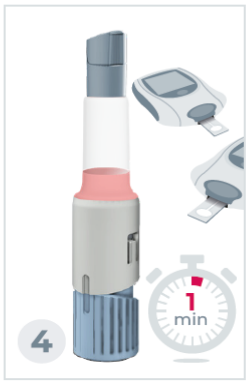

Let stand in upright position for 1 minute. Prepare instruments for testing according to method A or B.



Repeat step 3.








Method A
Sampling with dropper tip


2 min

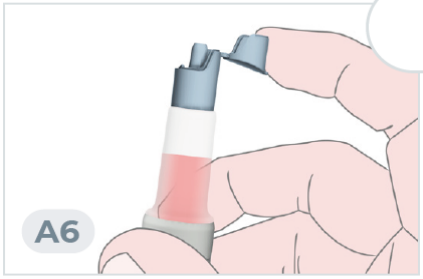

Open the cap when holding the device in an upright position.



Immediately discard first drop by squeezing transparent part.

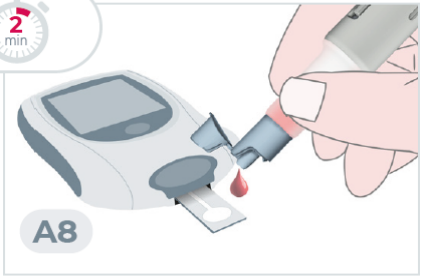

Apply a sample for testing.

Method B
Sampling with syringe

2 min



With cap in downward position screw the syringe on the luer adaptor.



With cap in upright position draw your sample and unscrew the syringe.



Immediately discard first drop and apply sample for testing.



Watch the Video Clip