

Participant Code replaces Lab Code.

Participant Code: WQ00000
 #####
 #####
 #####
 #####
 #####




Unit 6, Parc Ty Glas
 Llanishen
 Cardiff
 United Kingdom
 CF14 5DU
 Tel: 02920 314750
 Email: office@weqas.com
 Programme Organiser: Mrs Annette Thomas

Distribution details and report status.

Programme: **POCT INR** • Distribution Code: **IN0922**
 Distribution Start: 13-Sep-2022 • Distribution End: 11-Oct-2022 • Report Issued: n/a • Report Status: n/a
 Requested By: #####

Your % Poor PI (Performance Index) across all samples for all instruments, the Median All Participants % Poor PI and the 97.5th Centile % Poor PI.

| This Distribution | |
|--------------------------------------|----|
| Your % Poor PI | 0% |
| Median All Participant % Poor PI | 0% |
| 97.5 th Centile % Poor PI | 0% |

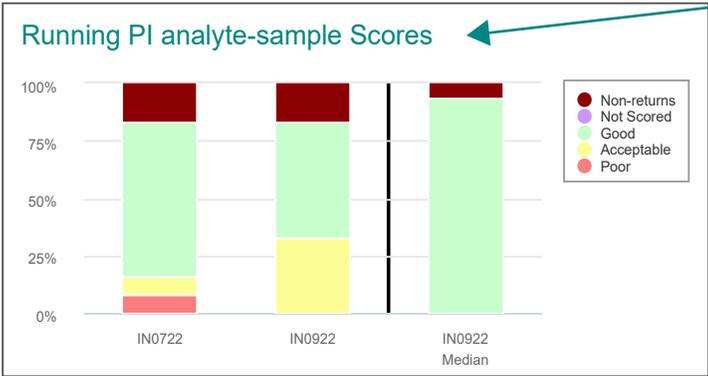

| PI Ranges | |
|-----------|------------|
| <1 | Good |
| 1-2 | Acceptable |
| >2 | Poor |

The running table shows the current distribution PI scores, and ultimately the previous 5 distribution PI scores for all analytes, for your Participant Code, plus all-Participant Median performance.

The PI Scores table shows performance for all analytes and all instruments.

| Location | Instrument Serial # | Instrument Name | INR | Overall % Poor PI | Overall % Non-Return |
|----------------------|---------------------|-----------------|------------|-------------------|----------------------|
| Anti-Coag Clinic | TZ1000001 | | Good | 0% | 0% |
| | TZ1000002 | | Acceptable | 0% | 0% |
| Day Surgery Unit | TZ1000003 | | Good | 0% | 0% |
| Endoscopy Unit | TZ1000004 | | Good | 0% | 0% |
| Ward 1 | TZ1000005 | | Acceptable | 0% | 0% |
| Ward 2 | UQ0000001 | | Acceptable | 0% | 0% |
| Pathology 1 | UQ0000002 | | Good | 0% | 0% |
| Ward 3 | TZ1000006 | | Good | 0% | 0% |
| Ward 4 | TZ1000007 | | Acceptable | 0% | 0% |
| Ward 5 | UQ0000003 | | NRR | 0% | 100% |
| West Building | TZ1000008 | | NRR | 0% | 100% |
| West Building Ward 1 | U00000004 | | Good | 0% | 0% |

Overall % Poor PI across all analytes for each instrument, and Overall % non return for each instrument.

PI scores are converted into performance categories and colour coded.

Key for PI Codes.

| PI Code | Meaning |
|---------|--|
| N/A | Not enrolled for this analyte |
| NRR | Analyte enrolled but no results returned |
| N/S | This quantitative analyte not scored for this distribution |

******* Please note*******
 The NQAAP expects 100% compliance on EQA returns. If you are enrolled for an analyte and have not returned a result (denoted by NRR in your PI table), this will be treated as a poor performance score. Please let us know as soon as possible if you are no longer providing this analyte as part of your diagnostic service.

Distribution Specific Comment
 There is no specific comment for this distribution.

Distribution Specific Comments from Weqas or participant.

| Participant submitted comments | | |
|--------------------------------|----------------------------|---|
| Location | Instrument Name / Serial # | Distribution specific comment from the participant |
| West Building | TZ1000008 | ANALYSER NOT IN CLINICAL USE - AWAITING TRAINING FROM ROCHE |

'Your reported result' will be shown in the units entered, in the Weqas standard units (if units entered are different from the Weqas standard units), and method corrected result (if appropriate for the analyte).

This will show whether you have been scored against Reference Value, Method Mean or Overall Mean and the actual target value will be shown here.

Running Performance chart shows the PI (Performance Index) score for each sample for the current distribution and the last 5 distributions, with colour coding for each performance category.





Overall Performance is shown as a 'Traffic light', with performance colour coded to easily identify the performance category.

Programme: POCT INR • **Distribution Code:** IN0922
Distribution Start: 13-Sep-2022 • Distribution End: 11-Oct-2022 • Report Issued: • Report Status: n/a

Participant Code: WQ00000 • **Location:** Anti-Coag Clinic • **Analysed Name:** n/a • **Serial #:** TZ1000002
Date Samples received: n/a • Date of Analysis: n/a • Operator Details: n/a • Storage Conditions: 2 - 8 °C

Analyte: INR • **Method:** CoaguChek Pro II • **Kit:** na

| INR (units) | |
|--|----------|
| | Sample 1 |
| Your reported result (units) | 1.9 |
| Your results are scored against: (Method Mean) | 2.073 |

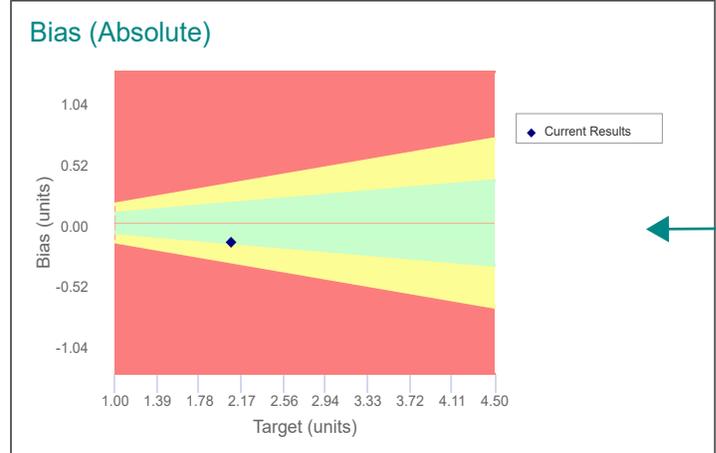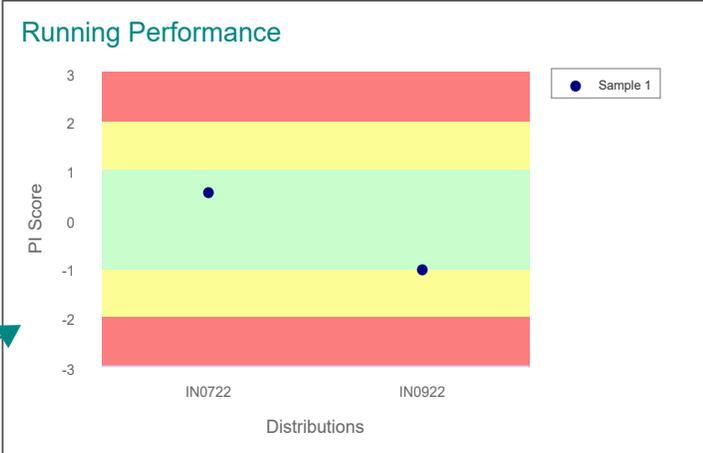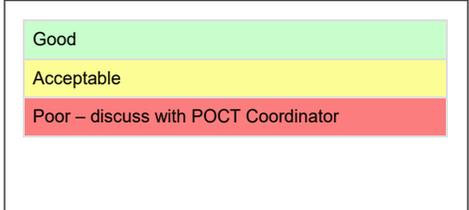

Your overall performance for this analyte is: **Acceptable**

- Your results for this distribution are acceptable

There are no Weqas or Participant supplied comments for INR for this distribution.

The individual Location and instrument details will be shown here.

The Bias (Absolute) Plot shows absolute bias in Weqas standard units for each sample for the current distribution. The x-axis is the target value; if the target value is a Reference Value or the Overall Mean, your Method Means will be plotted.

Overall Performance is stated here along with a basic interpretation of your performance and potential error identified.

Analyte Specific Comments from Weqas or participant.